

This instruction applies to the following item:

REF 2094

## To Install:




(1.) Place bottom end of support leg at foot of articulator.




(2.) Rotate support leg up to clip or attach to vertical support of the articulator.

## To Remove:

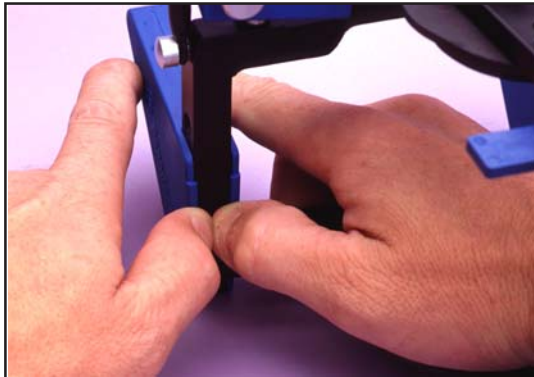


(3.) Place thumbs on retention clips.

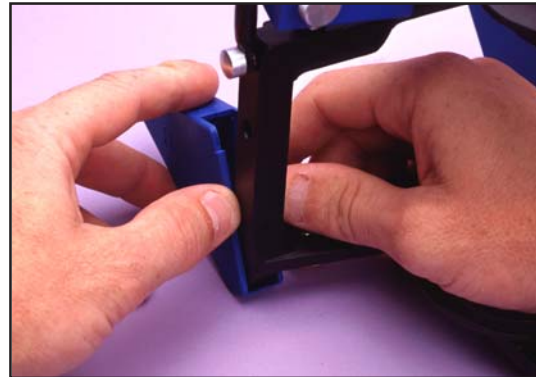


(4.) Push clips laterally and back to remove.

## To Use:

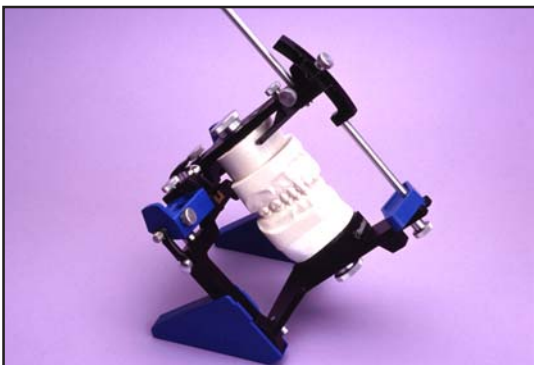

(5.) The Legs will support the articulator back 45° Degrees for patient consultations and photography procedures.

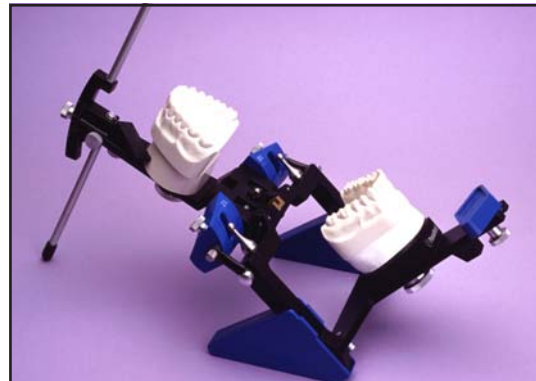

(6.) Open upper frame back to be supported by the support pin to facilitate laboratory procedures.